Clinical Comparison of a Generic Electrode Grid with Targeted Electrodes in Lower Limb Prostheses: A Preliminary Investigation

Ian Burford, Prosthetist Resident
Resident Directed Study
Shirley Ryan Abilitylab
6/21/17

As more research has begun to investigate the use of EMG data in the function of lower limb prostheses, it is important to understand fully the influence of electrode placement on the quality of EMG data. The previous studies on EMG control for lower limb prosthetic applications have yet to compare targeted electrodes and generic electrode grids. This study seeks to investigate the performance of a novel EMG system using a grid electrode pattern in comparison with a conventional EMG system using a targeted electrode pattern. The generic electrode grid system utilized in this study was the Mechanical Electrical Interface (MEI) system developed at the Center for Bionic Medicine (Reissman, Halsne, Lipschutz, Miller, & Kuiken, 2015). In this system, the electrodes were integrated into a gel liner during the fabrication of the gel liners and were linked to a custom attachment on the distal end of the gel liner. The distal attachment included magnets that coupled with magnets in the distal end of the socket, providing both suspension of the prosthesis and an interface for the internal electrical circuitry. The targeted electrode system used commercially available electrodes, MyoWare Muscle Sensor electrodes, to allow for comparison of muscle signal quality obtained by the two electrode systems. The targeted electrode system also utilized a gel liner and distal custom attachment. As the MyoWare electrodes included onboard circuitry, the distal attachments for the targeted liners did no

the MEI distal end connector was only used for suspension purposes since the electronic components were contained within the MyoWare sensors. Each subject was fit with a separate gel liner for each condition. Both subjects utilized an Otto Bock 4C for each condition, and the C-leg settings were tuned to each subject for optimal gait mechanics. A single prosthetic socket was fabricated per subject and used for both of the electrode conditions.

custom gel liner was fabricated with the electrodes and lead wires inside the gel of the liner creating 8 bipolar muscle signal recordings. This condition utilized the full MEI system. EMG data was amplified and recorded at 1000 Hz.

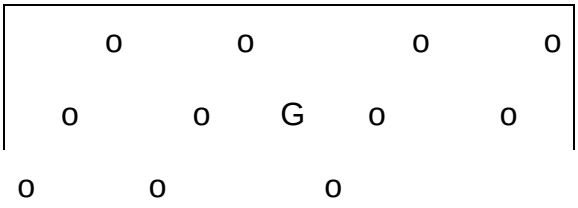

Discussion

EMG Issues

It is a difficult task to eliminate motion artifact from the EMG signals of a transfemoral limb while the subject is walking. Both the MEI and MyoWare EMG systems recorded various amounts of motion artifact during walking with a passive leg. For both systems, the motion artifact peaks seen in Figures 6-3 at Heel Contact and Toe Off were most likely created by the subjects pistoning inside the prosthetic socket as they walked. However, what is unknown is whether the motion artifact was occurring between Z t o] v Œ v š Z • µ i š [• • l] v } Œ the socket and the outside surface of the liner.

activation for all four channels.

Conclusions & Significance

The goal of this research study was primarily to perform an initial comparison between the performance of an electrode grid system and a targeted electrode system in a prosthetic setup. This study showed that both electrode systems were capable of detecting repeatable muscle patterns but that there is still improvement required to reduce the amount of motion artifact captured during EMG data collection. Additionally, this study revealed that there are various clinical challenges associated with incorporating either a novel electrode grid system or a conventional targeted electrode system into gel liners. These clinical challenges make it difficult to reliably and efficiently obtain useful EMG data for use with prosthetic devices. While

Design and Evaluation of a Cable-Driven, Body-Powered Orthosis for Individuals with Spinal Cord Injury

A Prosthetic Resident Research Project

Theresa Field, CPO

Resident Prosthetist, 2015-2016

Introduction

Spinal cord injuries occur when any damage has been done to the spinal cord.[1] Spinal cord injuries may be classified as complete or incomplete and temporary or permanent.[2] Thirty one percent of spinal cord injuries are at the cervical level; further broken down to 14.8% at C5, 11% at C6, and 5.4% at C7, as reported by King.[3] A spinal cord injury at the cervical level will result in a certain degree of loss of function of the upper extremity, requiring an assistive device to help improve grasping techniques for functional independence.

Typically, a person with a SCI at C6 or C7 level has the ability to operate a wrist driven flexor hinge orthosis (WDFHO) to complete various activities of daily

3. Harness

As previously mentioned, the harness design uses features of a standard transradial Bowden cabling system and also went through a few variations (Figure 3). Due to limited range of motion for persons with a spinal cord injury, there was concern that a Figure of 8 harness would be too difficult to don. A figure of 9 harness was trialed with a TRS Elf Strap. Unfortunately, the Elf strap did not provide enough support for the cabling system, so a figure of 8 harness was required. Initially, a northwestern ring was used but the straps slid around the ring too much. So, a TRS Baha buckle was used, which was more successful than a northwestern ring.

A functional prototype is pictured in Figure 4a; however, this version has no wrist joint. Figure 11b shows subject SCI 2 wearing this device and opening the thumb. The final device design used by subjects in the study had a wrist joint and a Baha buckle.

Functional Evaluation of Orthosis

Methods

The plan was to recruit up to 5 able-bodied subjects for design development—taking outcomes to help establish “normative data.” Then the plan was recruit 2 subjects with SCI to continue with design development. Finally, up to 5 more SCI subjects were to be recruited for outcomes measures. Two outcomes measured were decided upon, by a process of elimination, based on the goals of the study: the Box and Blocks test and the Jebsen-Taylor Hand Function test were selected to best assess device function. Both measures have been tested on the spinal cord injury population and both have normative data associated with them. Box and Blocks is recommended for use for the spinal cord injury population [5]. Jebsen-Taylor is reasonable to use in research for a person 3+ months post injury [6] As the orthosis was being tested in the lab at RIC, quality of life outcomes were disregarded; however, these issues can be evaluated in further trials.

Results

re died subjects fore distin-Ta in Bloa asse

To determine where the optimal thumb positioning should be, the Box and Blocks task was performed with the orthosis in two positions, thumb to pointer and thumb to pinky (Table 1). Most of the able-bodied subjects preferred the thumb to pointer position. Their feedback provides future design considerations and will be discussed in the next section. Subject SCI 2 was able to gather more blocks without wearing the assistive device (Table 2). This was due to the thumb shape and indicates that further device modifications are necessary. The Jebsen-Taylor task could not be performed due to the poor thumb design.

Table 1: Number of blocks moved in 1 minute by able-bodied subjects using each orthosis option

Subject	Thumb to Pinky	Thumb to Pointer
AB 1	8	9
AB 2	13	16

Future Work

All though the design requires further development, recruitment for this study was significantly difficult, which begs the question, is there a population to use this orthosis? The size of the prototype thumb needs to be shrunk down to a more anatomic size. The main future design considerations are making the thumb stationary yet prepositional and having the pivot point be at the MCP. The thumb must reflect an anatomical size thumb otherwise, grasping objects is too challenging for the patient. Since every person is different, it would be ideal to have the anchor of the thumb adjustable. Having stability in the coronal and sagittal planes would be ideal for proper function. The adjustability would allow for more productive fitting appointments prior to making a definitive orthosis.

Work Cited

1. Staff, M.C. Spinal Cord Injury 2014 2015 [cited 2015 May 15]; Available from: http://www.mayoclinic.org/diseases-conditions/spinal-cord-injury/basics/definition/con-20023837
2. Wood-Dauphinee, S., et al., Quality of life in patients with spinal cord injury--basic issues, assessment, and recommendations.

Localization of residual limb muscles of individuals with a transfemoral amputation and intact limbs

A Prosthetic Research Resident Project

Sara Hutchinson, CO, MPO, MS,
Prosthetic Research Resident, 2017
Shirley Ryan AbilityLab
Center for Bionic Medicine

Background

Most current commercially available transfemoral prostheses utilize passive knee and ankle components. While passive components are more common, there are some powered lower limb prosthetic components that are commercially available including the Ossur Power Knee and the BionX BiOM ankle. These components include mechanical sensors (i.e. load cells, inclinometers, inertial motion units, etc.) to determine when powered assistance should be provided. Using powered components can enable people to walk with increased gait efficiency by providing net positive work similar to muscles in intact limbs. Powered components can perform the majority of the work while ascending stairs step over step and ascending ramps. These benefits may translate into reduced joint damage over time. Research is currently being done to develop new powered knee and ankle components as well as improve the control of these components. One method of improved control may be the addition of inherent muscle sih8.1(a8lsJ -21.

currently involves dissecting the major nerves two to four centimeters proximal to the cut end of the bone. The quadriceps muscles are detached just proximal to the patella to retain some of the tendinous portion. The medial hamstrings are cut two to two and a half distal to the cut end of the femur, while the biceps femoris is transected at the level of the bone cut. The adductor magnus is first sutured to the lateral aspect of the residual femur via drill holes. The quadriceps are then sutured to the posterior aspect of the femur via posterior drill holes. The hamstring muscles are anchored to the posterior aspect of the adductor magnus or quadriceps.[6] In the Dundee technique, all muscles are retained at the level of the skin cut (~8cm distal to the bone cut). The adductors and medial hamstrings are sutured to anterior medial drills holes. Vastus lateralis and lateral hamstrings are sutured to anterolateral. The quadriceps are then brought over the end of the femur and attached to the hamstrings.[5] Surgical technique may vary for several reasons including surgical training, time of amputation and cause of amputation. In the case of a traumatic amputation, the surgeon may have less time to plan, less experience with amputations and/or damage to other structures within the residual limb. Based on the amputation method followed, muscle contraction strength, location and direction of pull may vary.

In addition to surgical technique effecting muscle belly location, thigh composition has been found to change in people with amputations with muscle decreasing and fat increasing following amputation.[7-10] Without hamstring fixation, the hamstrings experience 70% atrophy.

In addition to scaling the vertical muscle location by the contralateral trochanter to knee center measurement to simulate if the limb were intact, muscle locations were examined by scaling the vertical location by the residual limb length (Appendix K). When the vertical muscle locations were scaled by residual limb length for the subjects with a transfemoral amputation, there were no statistically significant differences between the vertical location and the vertical location scaled by trochanter to knee center of the subjects with intact limbs with the exception of VM (p=0.03).

Measurements of muscle locations while wearing a liner were not statistically significantly different from those found without a liner on with the exception of the vertical location scaled by residual limb length for ST (p= 0.01) (Appendix L). There was also a significant difference between the measurements taken from the distal end of the residual limb for ST and BF (p=0.01 and 0.02 respectively). The average donning variability for the three liner donning instances for all subjects across all muscles was 1.1 cm (0.9 cm horizontal, 0.5 cm vertical).

Discussion:

To our knowledge, this is the first study to report on generalized muscle locations in individuals with a transfemoral amputation.

Determining the area of greatest contraction was more difficult in subjects with a transfemoral amputation than it was in subjects with intact limbs. When palpating the subjects with a transfemoral amputation's residual limb the muscle location was sometimes shifted medially or laterally compared to what would be typical in an intact limb. Generally, when the muscles were shifted it was all of the quadriceps muscles being shifted in the same direction, which is likely due to surgical technique. It was also difficult for some subjects to complete the desired contractions, likely due to muscle disuse given the length of time since amputation. Having subjects complete the desired contraction bilaterally would sometimes improve the subject's ability to achieve the contraction. One subject also had scar tissue that made palpation of the area of greatest contraction more difficult. Subjects with more redundant tissue were also generally more difficult to palpate specific muscles. Even with these challenges, all of the desired muscles were able to be found with reasonable confidence. This process of determining muscle locations could be difficult and time consuming. Using the generalized muscle locations found in this study as a starting location would potentially decrease difficulty in targeting muscles in people with a transfemoral amputation.

Generalized muscle locations were able to be determined with increased variation in muscle location in the vertical direction compared to the horizontal direction when measuring from the greater trochanter. It was noted when taking measurements while the subject was wearing a liner that the vertical muscle location was often located in the area of the seal on the seal-in liner. This observation along with the potential future application of our data for the

Muscle locations were also examined while subjects with a transfemoral amputation were wearing an Ossur Iceross Seal-In liner. There were no statistically significant differences in horizontal location between measurements with and without the liner on. Hamstring muscles showed variation in vertical location in several of the measurement techniques. This variation could be attributable to the method of donning that could bring the posterior tissue more proximal as the liner is rolled up. The marks ma

Appendix C: Limb measurements for subjects with a transfemoral amputation.

	Contralateral limb measurements	Residual limb measurements			
Subject ID	Trochanter to knee center (cm)	RL length (cm)*	% limb remaining*	Circumference at horizontal reference (cm)	Distal circumference (cm)
TF1	42.5	24	56%	43	37.5
TF2	41.5	24.3	58%	42.9	39.5
TF3	41	26	63%	34	24
TF4	41.5	27	65%	45.2	41
TF5	41.5	27.8	67%	47.7	33.4
TF6	42	29.5	70%	46	41
TF7	52	37.8	73%	53.3	36
TF8	39.8	29	73%	48	43.8
TF9	36.2	30	83%	49.3	39

Appendix E: Area of greatest contraction for all six muscles (RF, VL,VM, ST, BF, and AM) of all subjects with a transfemoral amputation referenced to the greater trochanter.

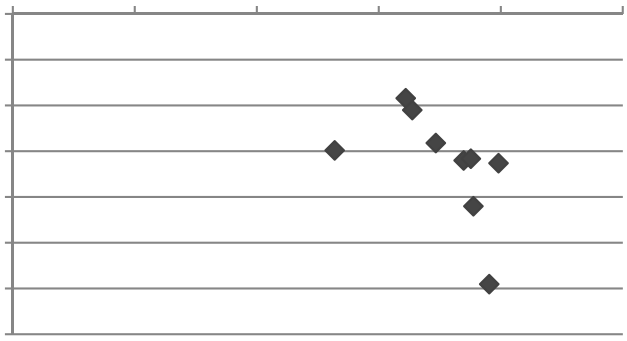

Appendix F: Average location of the area of greatest contraction for subjects with a transfemoral amputation.

Appendix G: Area of greatest contraction for all six muscles of all subjects with a transfemoral amputation referenced vertically from the distal end and horizontally from the greater trochanter.

Appendix H: Pearson correlation values between vertical location of the area of greatest contraction and limb length measurements.

Correlations between vertical muscle location and:	RF	VL	VM	ST	BF	AM
Contralateral trochanter to KC length	0.69	0.66	0.61	0.74	0.73	0.84
Uncompressed residual limb length	0.94	0.94	0.98	0.86	0.88	0.92
Compressed residual limb length	0.94	0.95	0.99	0.86	0.91	0.91

Appendix I: Sample plot for VM comparing residual limb length to vertical location of area of greatest contraction.

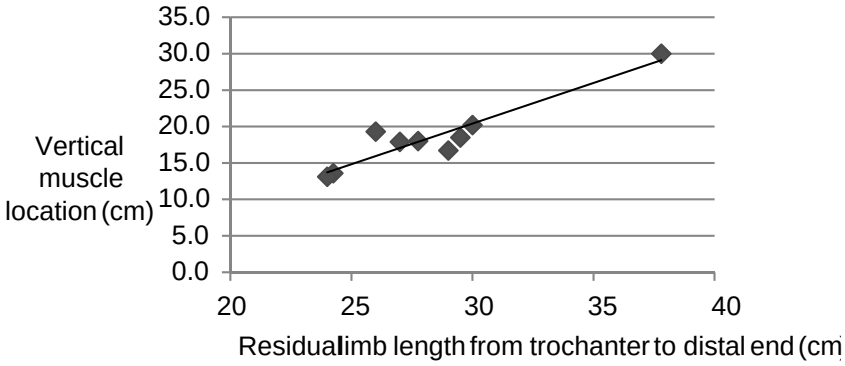

Appendix J: Scaled muscle locations for both subjects with a transfemoral amputation and subjects with intact limbs referenced to the greater trochanter. Horizontal locations are scaled by the horizontal reference circumference. Vertical locations are scaled by the distance from greater trochanter to knee center.

Appendix K: Scaled muscle locations for both subjects with a transfemoral amputation and subjects with intact limbs.

	Scaled location by:	RF_x	RF_y	VL_x	VL_y	VM_x	VM_y	ST_x	ST_y	BF_x	BF_y	AM_x	AM_y
Transfemoral	Contralateral KC	77% [4%]	38% [12%]	88% [7%]	43% [8%]	67% [5%]	42% [10%]	36% [6%]	48% [6%]	18% [8%]	48% [9%]	53% [7%]	33% [7%]
	Residual limb length	77% [4%]	57% [13%]	88% [7%]	64% [9%]	67% [5%]	65% [10%]	36% [6%]	73% [8%]	18% [8%]	72% [9%]	53% [7%]	50% [8%]
Able-bodied	Contralateral KC	78% [3%]	56% [6%]	90% [3%]	70% [5%]	64% [3%]	75% [8%]	38% [3%]	68% [5%]	17% [6%]	65% [8%]	54% [2%]	45% [7%]

Appendix L: Scaled muscle locations both with and without a liner on for subjects with a transfemoral amputation.

Outcome Testing of Two Commercially Available Myoelectric Hands with Wrist Rotation Units Using Pattern Recognition on Transradial Amputees.

A Prosthetic Resident Research Project

Ramen Landon, MPO, CTPO

may better allow amputees to perform many daily complex tasks like opening a lid of a jar or cutting food (3) (4) (5).

Multifunctional hands provide additional grip options for amputees, but being able to truly utilize the additional functions can be challenging, and the controls in these latest myoelectrical prostheses appears to be the weak link. For upper-limb amputees, there are traditionally very few ways to be able to control externally powered prostheses. If myoelectrical control is used as the input, then traditionally you would use direct control, a pair of electromyographic (EMG) electrodes placed over the agonist-antagonist muscle belly to control both directions of movement of the motor used in the prosthetic component. Additionally, other control strategies like co-contraction or double open can act as triggers or mode switches which can be utilized to alternate between multiple motors in the system but can be awkward for the user (6), (7).

Targeted Muscle Reinnervation (TMR) is another recent advancement that can assist in prosthetic control, where a broader spectrum of EMG information of additional individual muscle activity is made available but requires different control strategy to fully capture and take advantage of this added information (8). With TMR, nerves in the residual limb are redirected and transplanted to denervated donor muscle sites, which will reinnervate in time and provide new purposeful connections with the muscle they now control. The newly targeted muscles enable amputees to gain additional simultaneous control over prosthetic components (9). Even with this additional EMG data that TMR can deliver, traditional dual-site myoelectric controls are unable to fully harness this additional information and thus do little to help the users control the more complex multifunctional prosthetic hands effectively control multiple simultaneous movements (2).

One innovative and emerging prosthetic control system, called Pattern Recognition (PR), was developed to address some of the current short comings of traditional externally powered prosthetics. PR uses multiple EMG signals as well as algorithms to gather and classify the muscles activity. This additional EMG information, coupled with the PR algorithms, has the potential to allow the prosthetic user much greater control over higher DOF prostheses while also feeling more intuitive to operate (10).

With the introduction of TMR, PR and increasingly multiple-DOF devices, another challenge is K R Z E H V W W R T X D Q W L I \ W K H adYantages of these technologies. One way W R K D is to use a real-time virtual reality (VR) test that uses a multiple-DOF classifier that provides real-time closed-loop performance measures to capture how well test subjects complete them motions. One such test is the Target Achievement Control Test (TAC Test) (

device, users performed functional outcomes with each device and pre-study/post-study VR TAC testing.

The initial research study protocol and subject questionnaire were developed,

The test subjects were measured and fitted with an appropriate fitting glass silicone liner

deviate or lengthen the wrist/ hand with ease

Pictures along with documentation were used to capture the initial setup for each subject and much care was taken to ensure that the liner was donned in the same orientation and the correct PR color coded wire snaps attached to the corresponding electrode for each visit. In figure 3, an example PR Isetupnnd the

Subjects

Results

Lastly, the SHAP test has the subject perform 26 timed tasks, fourteen of which fall into ADL-like tasks and eight abstract object tasks repeated with light and heavy objects that can be classified into six prehensile patterns with an overall index of function score of 0 (minimum) to 100 (maximum) based on non-amputee controls (14). The SHAP had an average Index of Function Score of 29.67 ± 5.51 with the 1-DOF system, while the average MAH score was 19.33 ±5.77 (graph 3).

The Hand/Wrist Evaluation Questionnaire handout, along with the numbered responses in graph form for both 1-DOF and MAH on all three research subjects, can be found in Appendix A and B. Although the results on the surveys were insightful, they were never intended to be statistically relevant to this study. However, the subjects scoring and responses do give subjective information that can be useful in future research and developments.

Conclusions

Both the 1-DOF and MAH wrist/ hand systems could be controlled by & R D S W ¶ V commercially available PR system and subjects were able to perform all of the outcome tests. The multifunctional Michelangelo hand was more challenging to control for the test users, and this can be seen in the results of the timed outcome tests. There may be a couple reasons for this. We were working with early enhanced versions of the commercially available software for the Michelangelo hand and some minor software optimizations settings needed to be adjusted during the course of our testing which may have restricted the hand¶V full potential. One subject specifically struggled with the system during multiple sessions as this was resolved, which may have frustrated him enough to lose confidence in the system overall.

Some limitations in the study were

Bibliography

1. Ziegler-Graham K, MacKenzie EJ, Ephraim PL, Travison TG, Brookmeyer R. Estimating the

Appendix A.

SBIR Hand/ Wrist Evaluation Questionnaire

For administrative use only:

Study Staff Member: _____ Date survey completed: _____

Subject Code: _____

Comparison to your previous device(s):

_____

Please circle one: Lab trial ± 1 2 3 TD ± A B C

Test subject instructions:
Please complete the following survey based on your experience with the control system you have been using for the most recent test period. If you require additional room for your comments, please continue on the back of this survey.
Please answer the following questions by circling the number which most accurately represents your opinion, for example, circling #5 would indicate that you strongly agree with the statement. Selecting #3 would indicate no opinion.

1. The prosthetic hand responded as I expected

Strongly Disagree 1 2 3 4 5 Strongly Agree N/A
Comments: _____

2. I felt that I had to watch the hand when I was moving it.

Strongly Disagree 1 2 3 4 5 Strongly Agree N/A
Comments: _____

3. It was easy to make the prosthetic hand move when I wanted.

Strongly Disagree 1 2 3 4 5 Strongly Agree N/A
Comments: _____

4. There were a lot of unintended movements of the prosthetic hand.

Strongly Disagree 1 2 3 4 5 Strongly Agree N/A
Comments: _____

5. I was frustrated using the prosthetic hand.

15. I felt fatigued after using the system.

Strongly Disagree 1 2 3 4 5 Strongly Agree N/A
Comments: _____

16. I would like to continue to use this control at home.

Strongly Disagree 1 2 3 4 5 Strongly Agree N/A
Comments: _____

Additional comments:

_____

_____

_____

_____

_____

Following the final trial please answer the following questions:

I preferred

Please circle one: Lab trial ± 1 2 3

Please provide comments on why you selected this trial:

_____

_____

_____

_____

Appendix B.

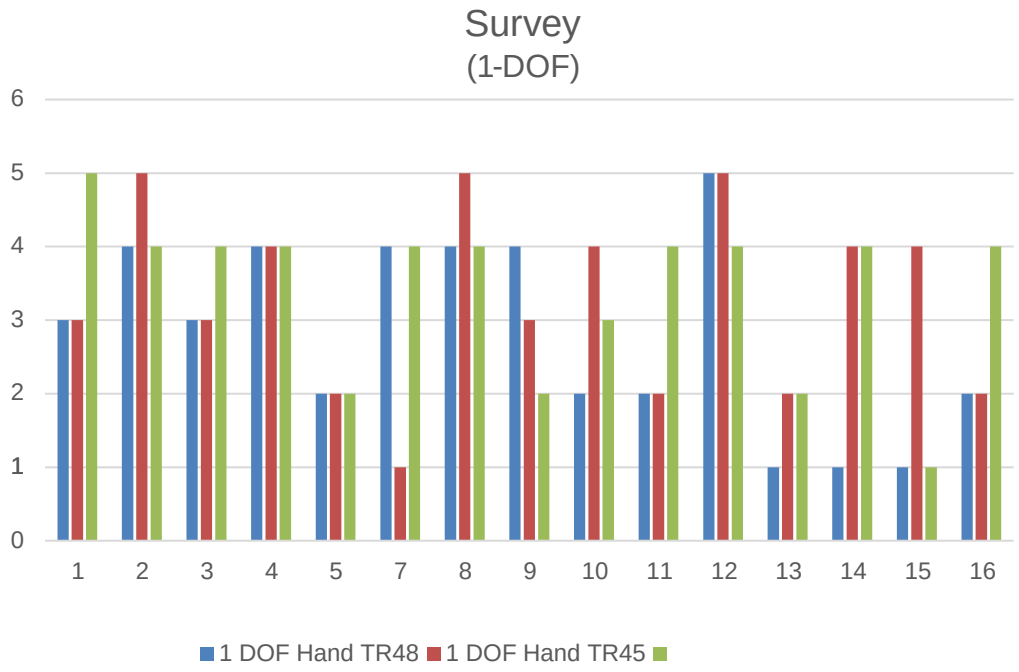
Survey
(1-DOF)
6
5
4
3
2
1
0
1
2
3
4
5
7
8
9
10
11
12
13
14
15
16
1 DOF Hand TR48
1 DOF Hand TR45

Development and Evaluation of a Novel Connector, the Magnetic Locking Interface (MLI), for attachment of a Lower Limb prosthesis

A Prosthetic Resident Research Project

Michael Socie, CPO

Resident Prosthetist, 2014-2015

Rehabilitation Institute of Chicago

Center for Bionic Medicine,

My prosthetic research residency project involved the development and testing of a novel connector to attach a lower limb prosthesis to the user. This connector, the Magnetic Locking Interface (MLI), attaches a lower limb prosthesis to the user through a prosthetic liner. Various types of connectors and locking

hope to publish the results of this study in a peer-reviewed journal. Additionally, we plan to present this work at 1 or more conferences that are relevant to the prosthetics community.